


△ 400 (300KV)
300 (210KV)
200 (160/225KV)
200 (100KV)

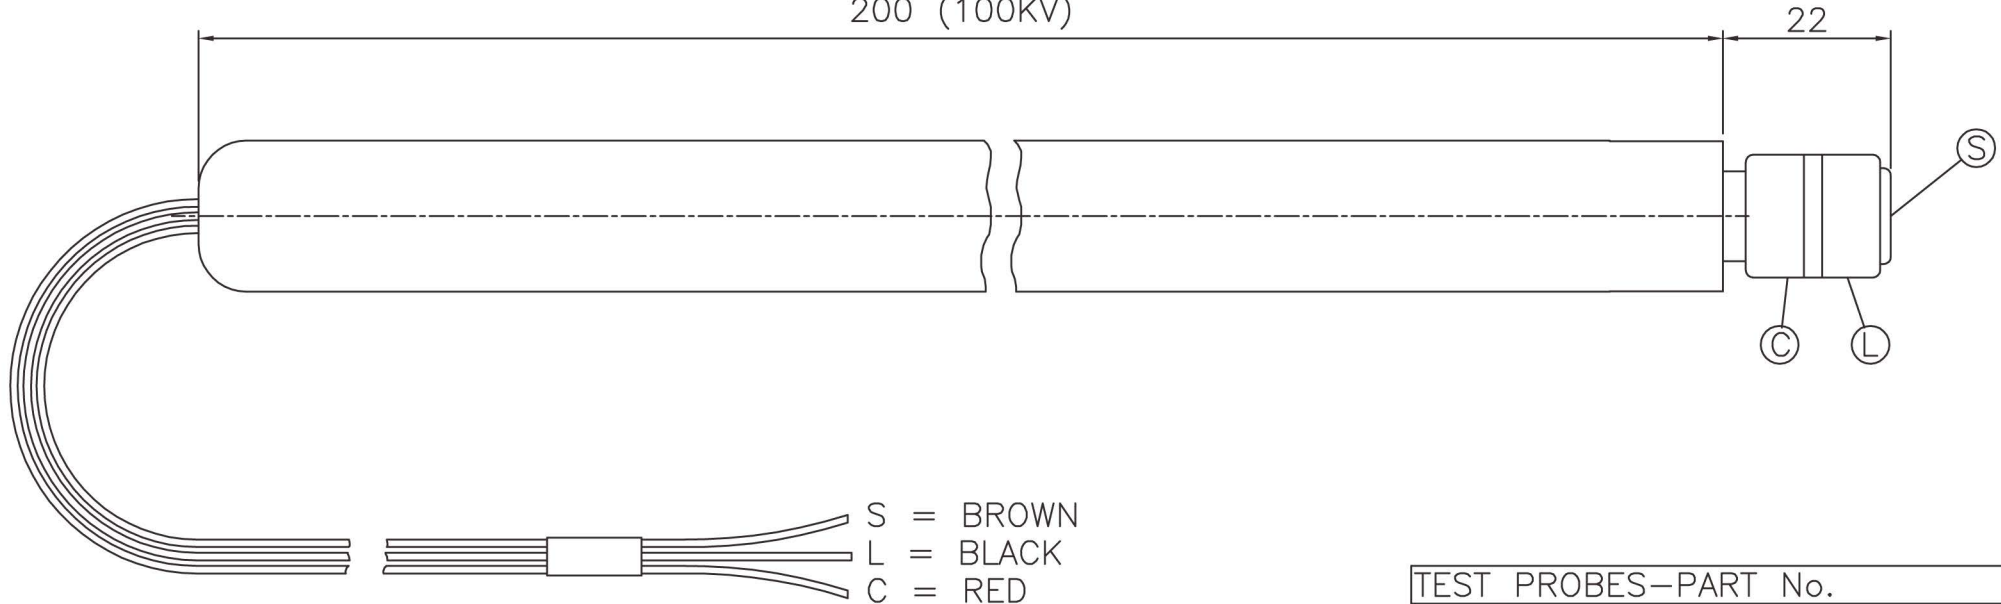

CABLE LENGTH APPROX 0.9M (300KV APPROX 0.75M) △

TEST PROBES-PART No.	
160/225KV	PART No. A93001
100KV	PART No. A93013
210KV	PART No. A93014
300KV	PART No. A93023

THIS DATA SHEET IS FOR IDENTIFICATION
PURPOSES ONLY. NOMINAL DIMENSIONS IN MM.

TECHNICAL DATA:

TERMINATION:
NOMINAL OPERATING VOLTAGE 240 VOLTS DC
CABLE LENGTH TOLERANCE +/- 100mm

ACCESSORIES:

INSTALLATION:

ESSEX

Dandong Light Electric Co.,Ltd
Rm.1606 Jiadi Square,No.64,Binjiang Middle Rd,
Zhenxing, Dandong, Liaoning China
T:0415-6123232
F:0415-6123533

REVISIONS

NO.	DATE	BY
5	21.05.02	DCN 1690
6	02.08.04	DCN 2035
7	02.02.05	DCN 2251
8	07.03.11	DCN 3183

DUE TO CONTINUING PRODUCT DEVELOPMENT ESSEX X-RAY RESERVES THE RIGHT TO MODIFY DATA WITHOUT NOTICE

DRAWN	APPROVED	DATE	ISSUE	SCALE
TSC		26.4.99	8	1:1

© NOT TO BE REPRODUCED IN WHOLE OR PART WITHOUT
PRIOR PERMISSION OF ESSEX X-RAY & MEDICAL EQUIPMENT LTD.

TITLE TEST PROBES

DRAWING No.

DS1036